

Rapid Digital Thermometer

Model:DT-K01A(Not Waterproof)



DT-K11A(Waterproof)

DT-K11B(Waterproof)

DT-K101A(Flexible tip, Not Waterproof)

DT-K111A(Flexible tip, Waterproof)

DT-K111B(Flexible tip, Waterproof)

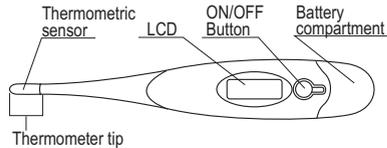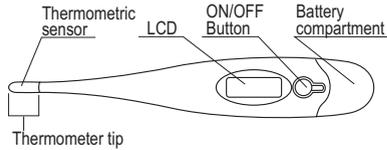

Note: The exterior of each model has a little difference.

Congratulations on your purchase of this product. Please read the instructions carefully before using the thermometer for the first time, and keep these in a safe place. This product is intended for the measurement of human body temperature. This product is for home and hospital use, operator shall be at least 11 years old and patient can be operator.

Operating Instructions

Before using, please disinfect the probe at first. To switch on, press the ON/OFF button next to the display; a short beep will sound, indicating that the thermometer is operational. At the same time the thermometer runs a self-check test, during which all the digital segments appear on the LCD. When the letters "Lo" and a flashing "C" or "F" display, the thermometer is now ready for use. If the ambient temperature is below 32°C or 89.6°F, then "Lo°C" or "Lo°F" will appear on the LCD and if it is more than 42.9°C or 109.2°F, then "Hi°C" or "Hi°F" will appear on the LCD. During the reading, the current temperature is displayed continuously and the "C" or "F" symbol flashes. The measurement is completed when a constant temperature value has been reached. The temperature value is considered constant when the temperature rises less than 0.1°C within 8 seconds. As soon as the constant temperature value is reached, a beep will sound ten times, and the "C" or "F" symbol will stop flashing. The highest measured temperature appears on the LCD. However, please note that this thermometer is a maximum thermometer, i.e. the displayed temperature can increase slightly if measurement continues after the beep. This is particularly the case with axillary measurements, the temperature value should be recorded which approximates the core body temperature. In this instance please note the description under "Methods of measuring temperature". When the measurement is completed, please switch the thermometer off by pressing the ON/OFF button. After the temperature has been displayed, the thermometer will shut off automatically after 10 minutes.

Memory function

Turn on the thermometer, the last measured temperature will display on the LCD for approximately 2s after the self-check. The reading will be over-written when the "C" or "F" flashes, i.e. the thermometer is ready for a next measurement, whether the new measurement is complete or not.

Methods of measuring temperature

It is important to remember that the body temperature reading depends on the site where it is measured. For this reason, the measurement site must always be Specified in order to ensure that a correct temperature reading is recorded.

In the rectum(rectal)

This is the most accurate method from a medical point of view, because it comes closest to the core body temperature. The thermometer tip is inserted carefully into the rectum for a maximum of 2 cm.

The usual measuring time is approximately 9 to 11 seconds.

Under the arm(axillary)

Placing the thermometer in the armpit provides a measurement of surface temperature that can fluctuate by around 0.5°C to 1.5°C from rectal temperature readings in adults. The usual measuring time for this method is Approximately 23 to 29 seconds. It should be noted, however, that an exact reading cannot be obtained if, for example, the armpits have been allowed to cool. If this is the case, we recommend extending the measuring time by around 5 minutes in order to obtain the most precise possible reading that corresponds as closely as possible to the core body temperature.

In the mouth(oral)

There are different heat zones in the mouth. As a general rule, the oral temperature is 0.3°C to 0.8°C lower than the rectal temperature. To ensure that reading is as accurate as possible, place the thermometer tip to the left or right of the root of the tongue. The thermometer tip must have constant contact with the tissue during the reading and be placed under the tongue in one of the two heat pockets at the back, keep the mouth closed during the reading and breathe evenly through the nose. Do not eat or drink anything before the measurement. The usual Measuring time is approximately 15 to 19 seconds.

Note: We strongly recommend the rectal method as the most accurate method for identifying the basal temperature, and advise you to extend the measuring time by 3 minutes after the beep.

How to change the measuring scale(only for switchable type)

To switch the display between °C and °F, turn the unit on. Press and hold the ON/OFF button for 2 seconds, the display will show another scale.

Cleaning and disinfection

The best way to clean the thermometer tip is by applying a disinfectant (e.g. 70% medical alcohol) with a damp cloth. It shall be disinfected before each use. The Waterproof thermometers can be immersed in liquid or lukewarm water for through cleaning and disinfection, but the Not Waterproof thermometers can not be allowed.

Safety precautions

- Do not allow the device to come into contact with hot water.
- Do not expose to high temperatures or direct sunlight.

- Do not drop the thermometer. It is neither shock-proof nor impact-resistant.
- Do not modify this device without the authorization of the manufacturer.
- Do not bend or open the device (except the battery compartment).
- Do not clean with thinners, petrol or benzenel. Only clean with water or disinfectant.
- Do not immerse the Waterproof thermometers under water 15cm for longer than 30 minutes.
- The thermometer contains small parts (battery, battery compartment) which can be swallowed by children. For this reason, do not leave the thermometer unattended in the hands of children.
- Avoid bending the Non-Flexible thermometer tip. For the Flexible thermometer, avoid bending the tip by more than 45 degrees
- If the ambient temperature is over 35 °C or 95 °F, dip the thermometer tip in cold water for approx. 5 to 10 seconds prior to measuring the temperature.
- Persistent fever, in particular in children, has to be treated by a doctor- please get in touch with your doctor!
- Do not use near strong electromagnetic fields, i.e. Keep it away from any radio systems and mobile phones.

Battery replacement

The battery is empty and needs replacing when the "▲" or "□" battery symbol appears on the right of the LCD. Remove the battery cover and replace it with a battery (preferably non-mercury) of the same type. Please note:

The "+" sign up and "-" sign down.

Product disposal

Please ensure environmental protection. Batteries do Not belong in the domestic waste. Please hand them in at collection point or the municipal recycle material Centre as special waste. The alkaline battery or fuel cell may lead to excessive temperatures, fire or explosion.



This symbol on products and/or accompanying documents means that consumed electronic products must not be mixed with conventional domestic waste. Take these products to the corresponding collection points for correct treatment and recycling, where they will be accepted free of charge. For more information on the closest collection point, Please enquire with your local authorities.

Technical data

Type: maximum thermometer

Measurement range:(32.0~42.9)°C/(89.6~109.2)°F

Measurement accuracy:

+/-0.1°C/0.2°F (35.5°C~42.0°C/95.9°F~107.6°F)

+/-0.2°C/0.4°F (32.0°C~35.5°C, 42.0°C~42.9°C /89.6°F~95.9°F, 107.6°F~109.2°F)

Storage/transportation temperature:

(-25~55)°C, ≤95%RH

Ambient temperature during use: (5~35)°C, ≤80%RH

Min Scale: 0.1 C/0.1 F

Battery type:

Alkaline battery, type LR41, 1.5V, service life

minimum 100 hours under continuous operation.

Weight: approx. 13g

Atmospheric pressure:700~1060hPa

Shelf life: 3 years

Explanation of symbols

▲ or □ battery is empty

⚠ Type BF equipment

♻ Product disposal instructions for electronic devices

LOT Lot number

⚠ Read IFU carefully

🏭 Manufactured by

CE CE conformity marking

📅 date

♻ The battery in this product complies with the requirements stated in European Directives 2006/66/EEC.

Lo°C or Lo°F: temperature under 32°C or 89.6°F
Hi°C or Hi°F: temperature over 42.9°C or 109.2°F

IP22 Classification according to the degree of protection against ingress of water as detailed in IEC 60529

Legal requirements and guidelines

This product complies with the European Directive for Medical Devices 93/42/EEC and carries the CE mark. The device also complies with the specifications of the European Standard EN 12470-3 Clinical thermometers-Part 3: Performance of compact electrical thermometers(non-predictive and predictive) with maximum device. The CE marking confirms that this is a medical device with a measuring function in the sense of the Medical Devices Act which has undergone a conformity assessment procedure. A Notified Body confirms that this product fulfils all the appropriate statutory regulations.

Calibration check

This thermometer is initially calibrated at the time of manufacture. If this thermometer is used according to the operation instruction, periodic re-adjustment is not required. The calibration check has to be carried out immediately, if there are indications that the product does not keep the defined error limits or the calibration properties could have been affected by an intervention or by any other means. Please also observe any national statutory regulations. The calibration check can be carried out by the competent authorities or by authorised service providers. A test instruction for calibration check can be provided to the relevant authorities and authorised services providers on request.

Warranty

This product is warranty for 1 year from the date of leave factory. Damage resulting from incorrect use or abuse is not covered by the warranty. Battery and packaging are excluded from the warranty. Claims beyond this, including claims for damages, are excluded. If you find that the thermometer is defective and not in good function, please firstly check the battery before sending in for repair. The manufacturer will make available on request circuit diagrams, component part lists, descriptions, calibration instructions, or other information that will assist service personnel to repair those parts of device.